



2 / 32

FIG. 2

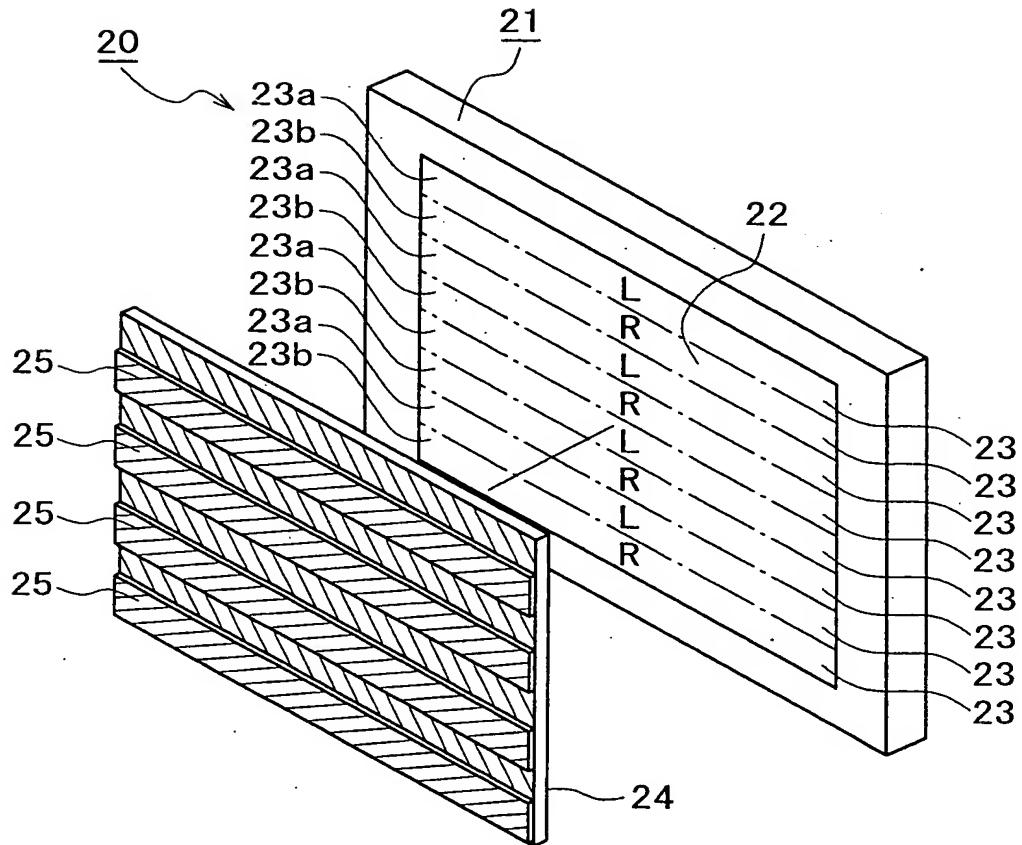


3/32

FIG. 3

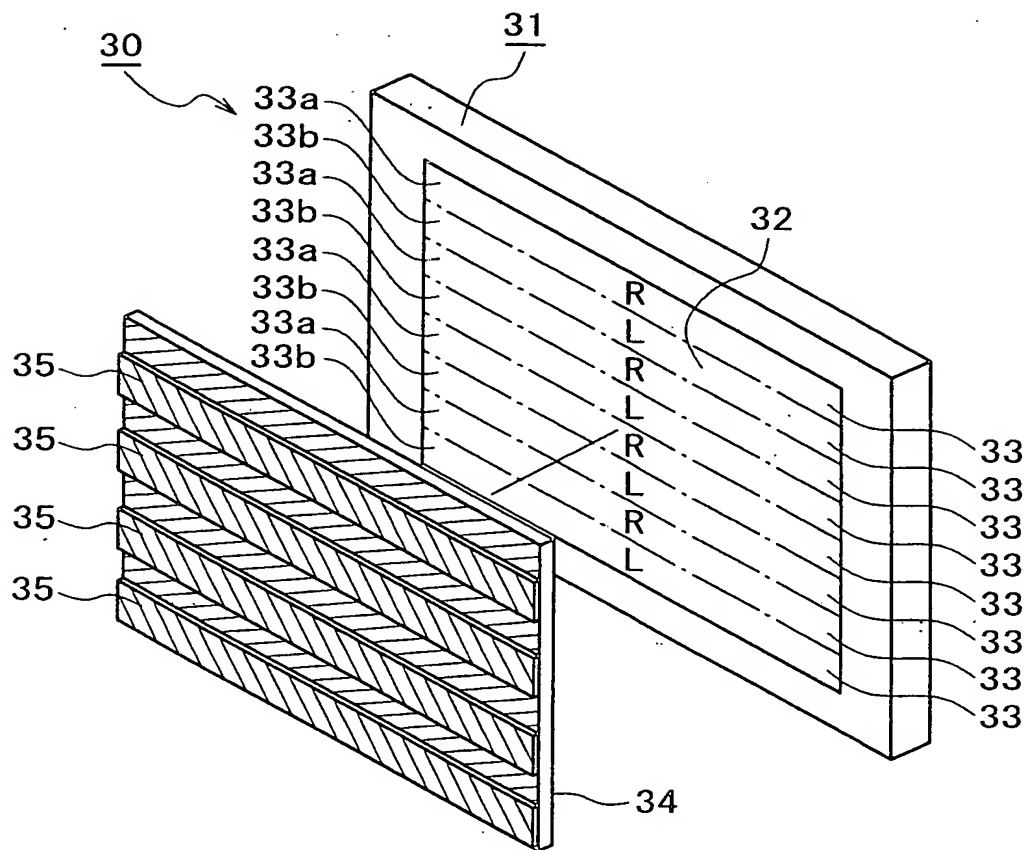


4 / 32

FIG. 4

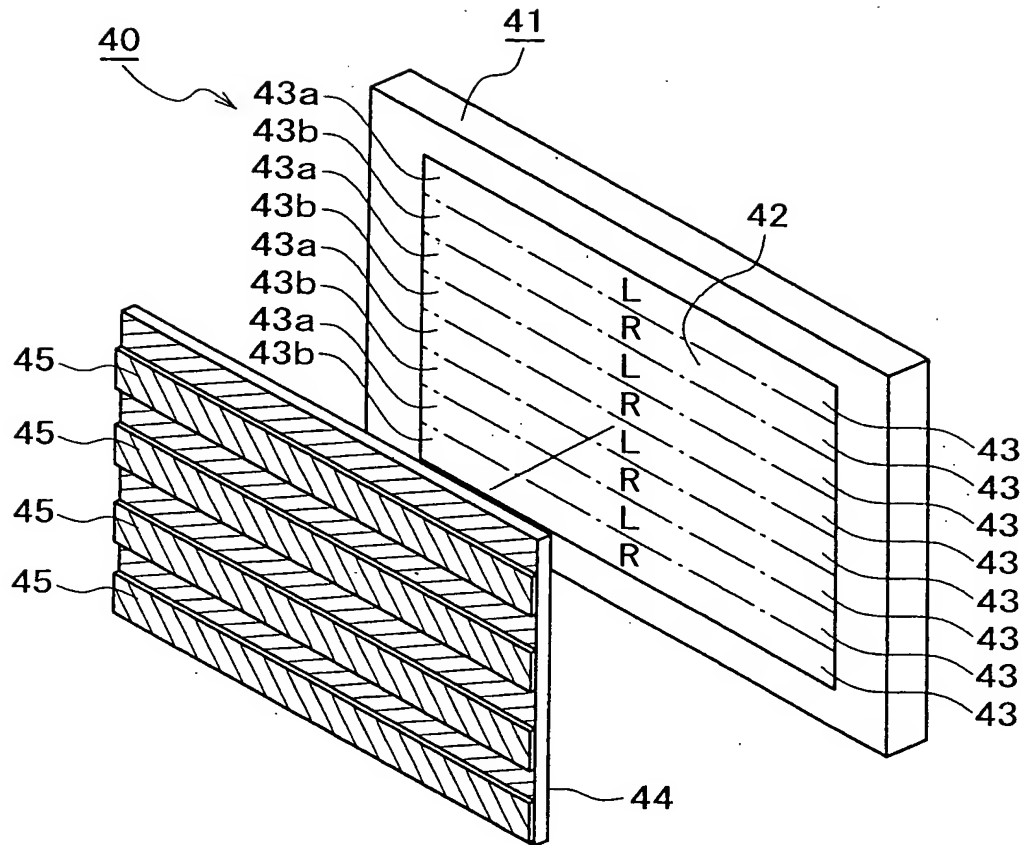


5/32

FIG. 5

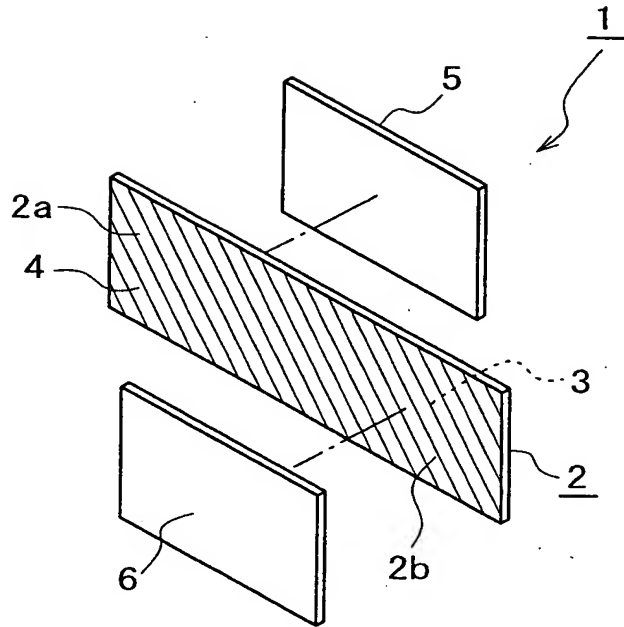


6/32


FIG. 6

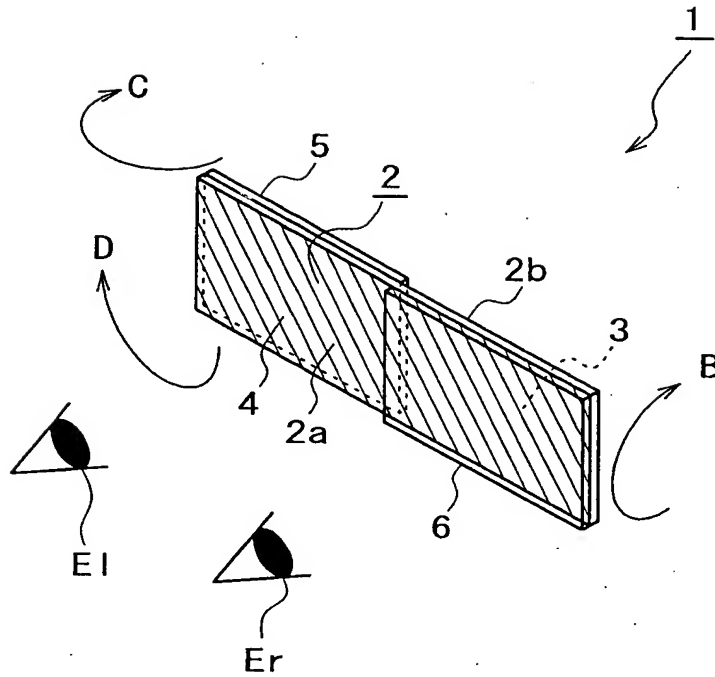

7/32

FIG. 7

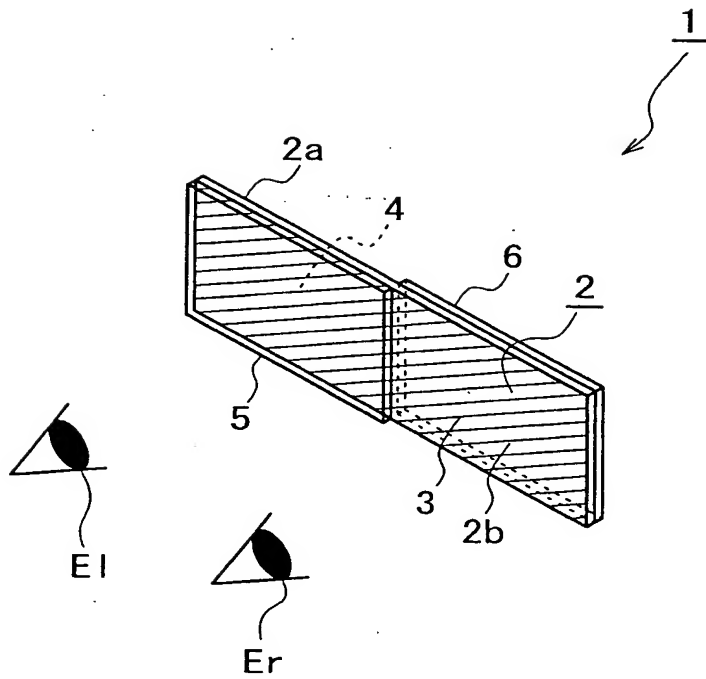


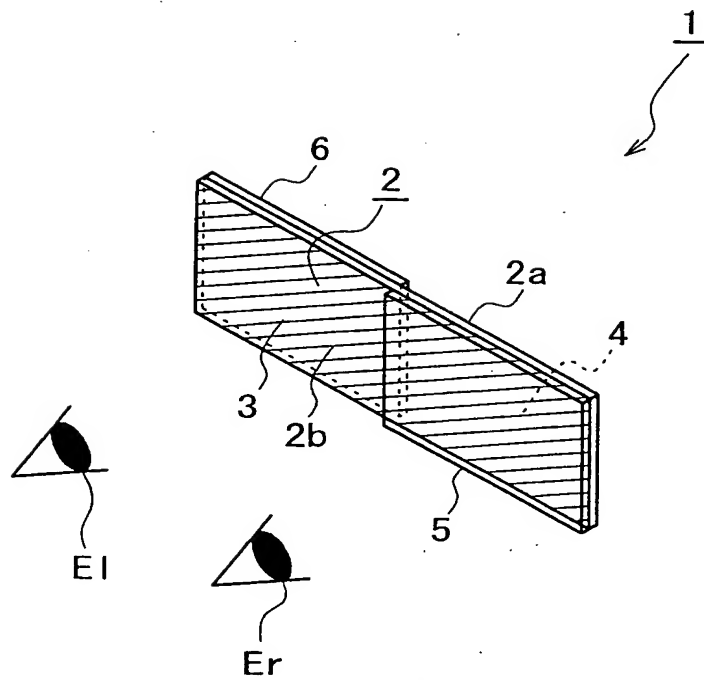



9/32

FIG. 9

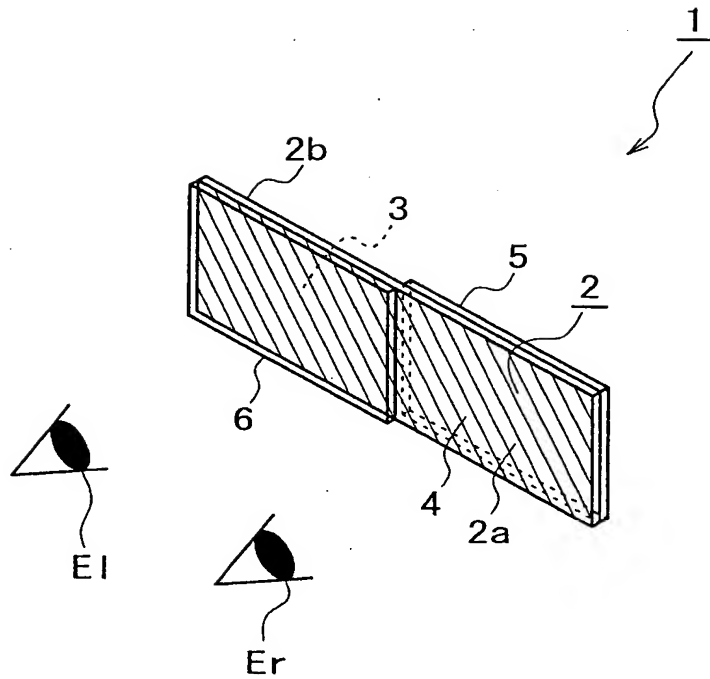




| STEREOSCOPIC IMAGE DISPLAY APPARATUS |         |          |         |  | POLARIZING EYEGLASS DEVICE |                     |                     |                     |
|--------------------------------------|---------|----------|---------|--|----------------------------|---------------------|---------------------|---------------------|
| TYPE I                               | TYPE II | TYPE III | TYPE IV |  | SERVICE CONDITION A        | SERVICE CONDITION B | SERVICE CONDITION C | SERVICE CONDITION D |
|                                      |         |          |         |  |                            |                     |                     |                     |
|                                      |         |          |         |  |                            |                     |                     |                     |
|                                      |         |          |         |  |                            |                     |                     |                     |
|                                      |         |          |         |  |                            |                     |                     |                     |
|                                      |         |          |         |  |                            |                     |                     |                     |

FIG. 11


12/32

FIG. 12

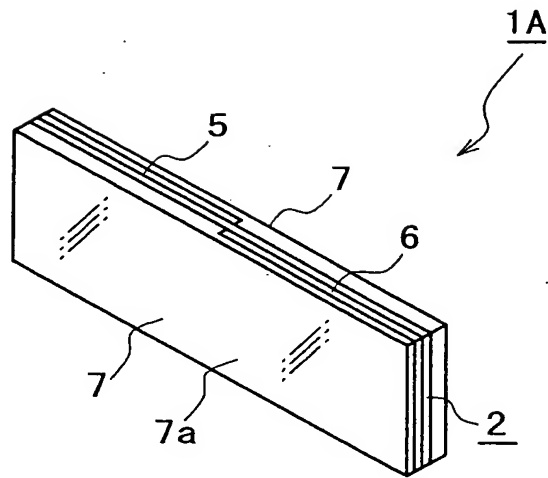


13 / 32

FIG. 13

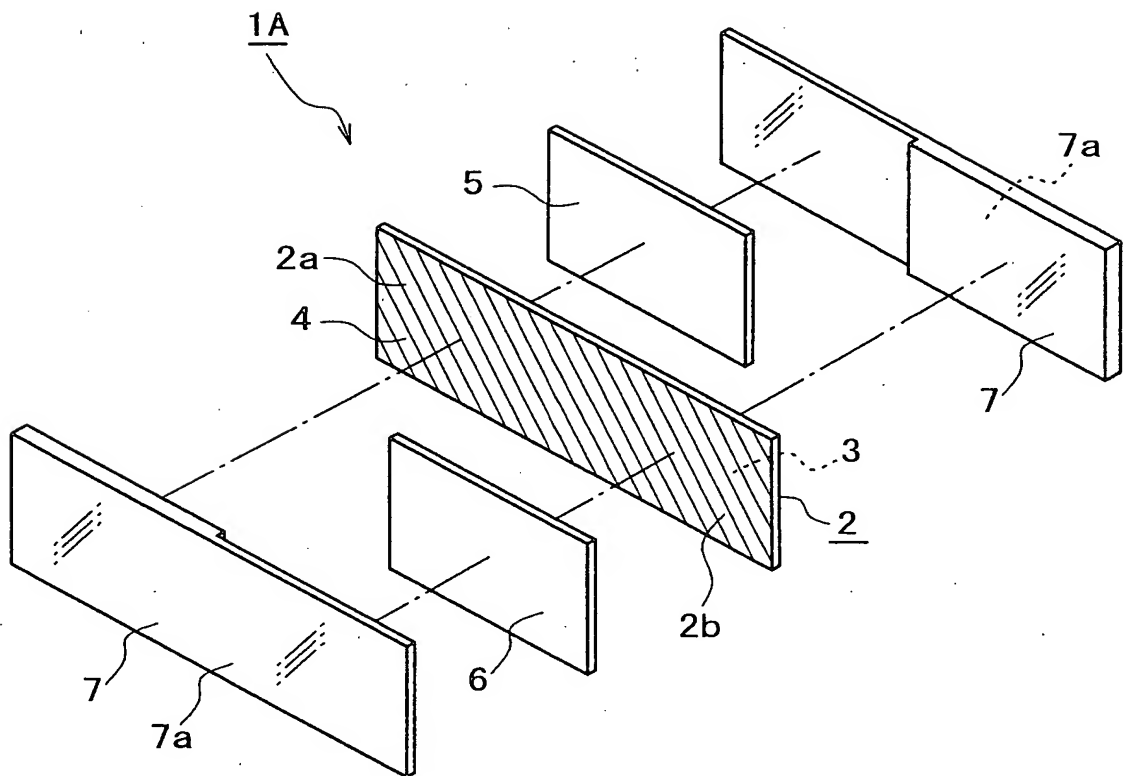

14 / 32

FIG. 14

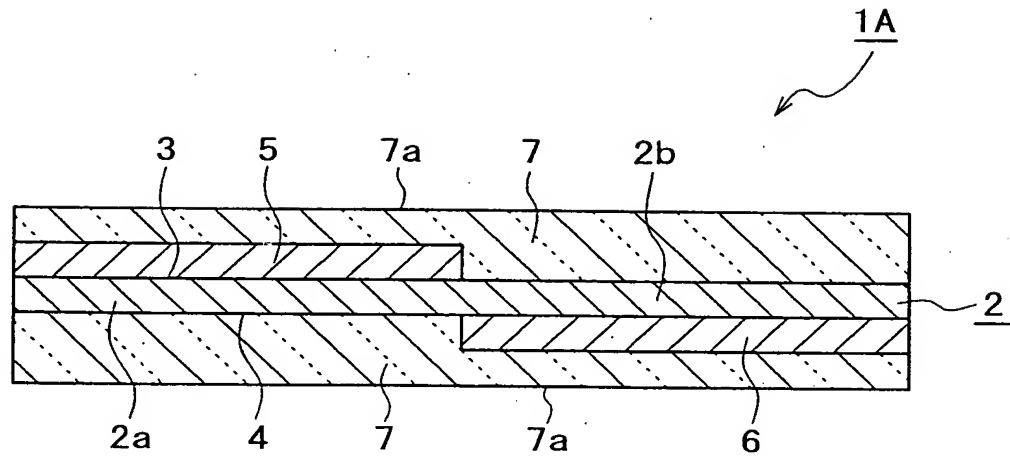

15/32

FIG. 15


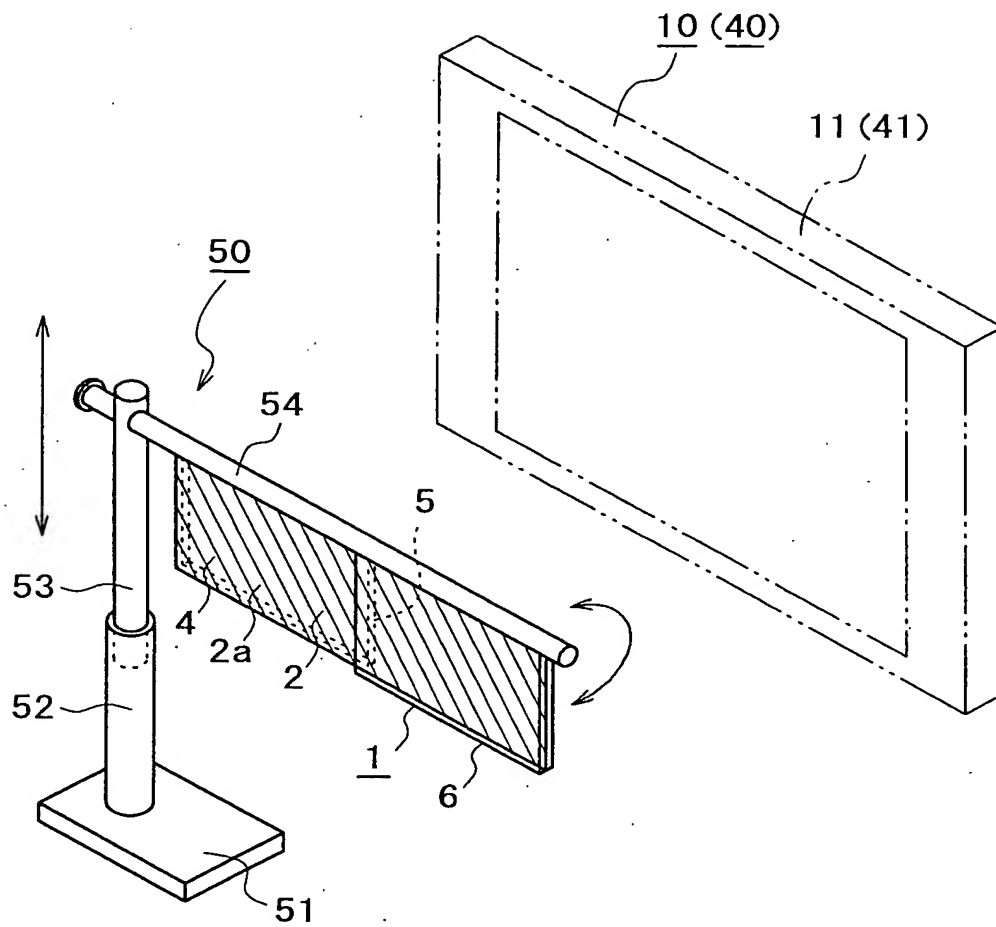



FIG. 16



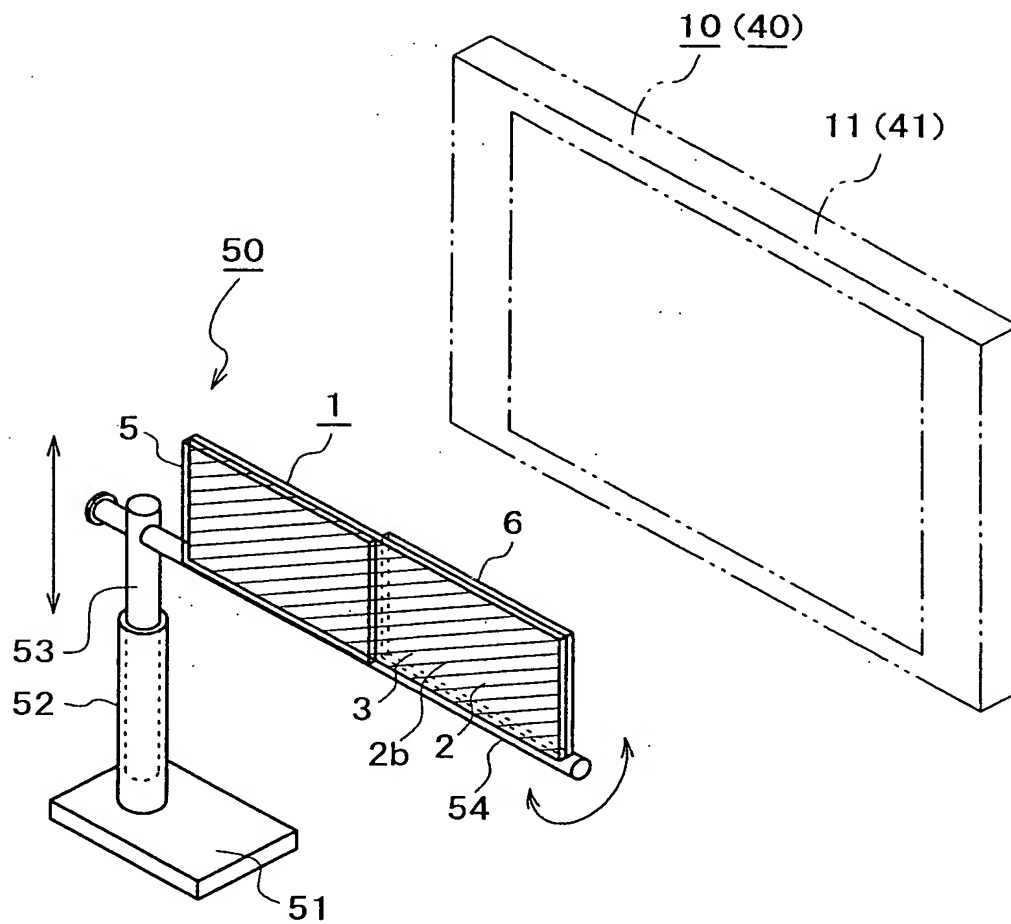


17/32

FIG. 17

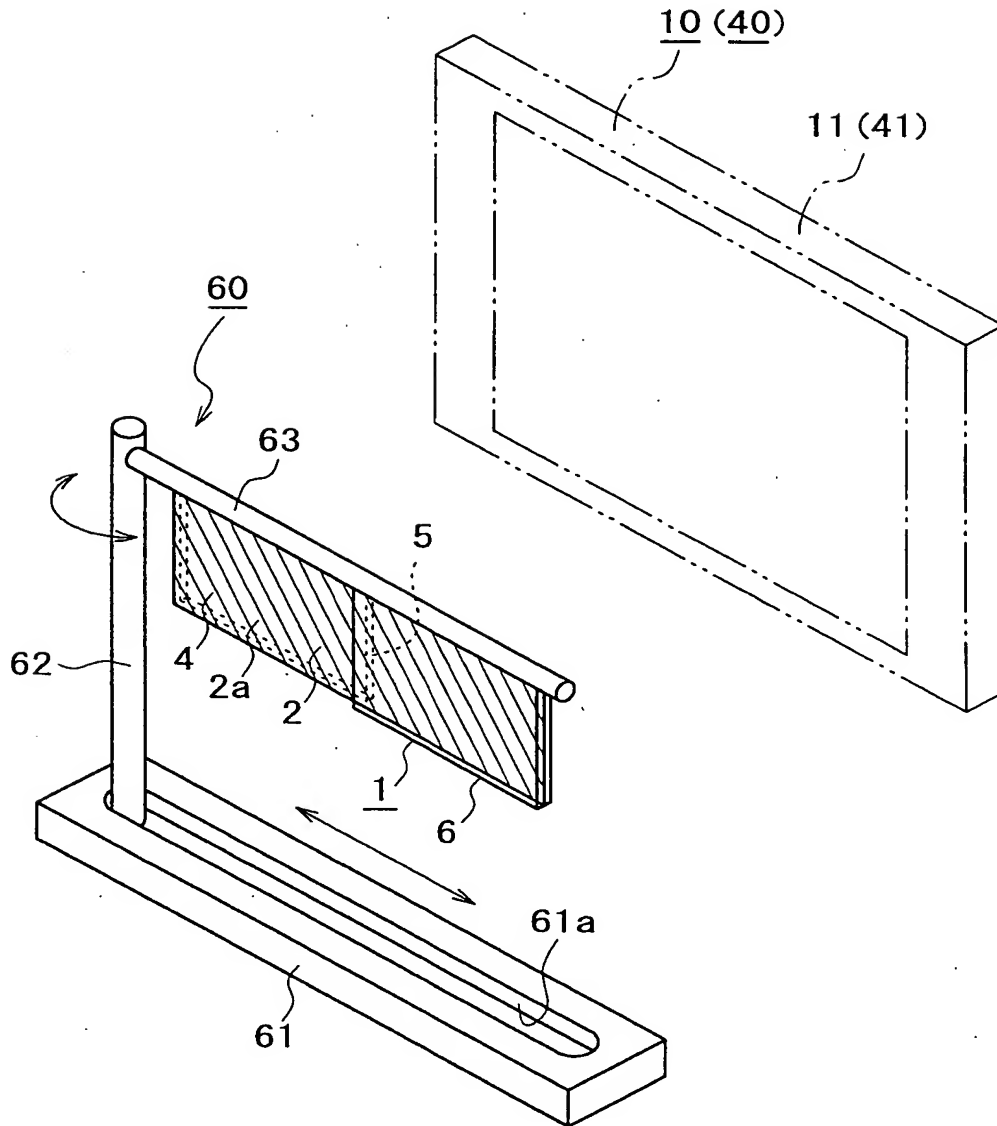

18/32

FIG. 18

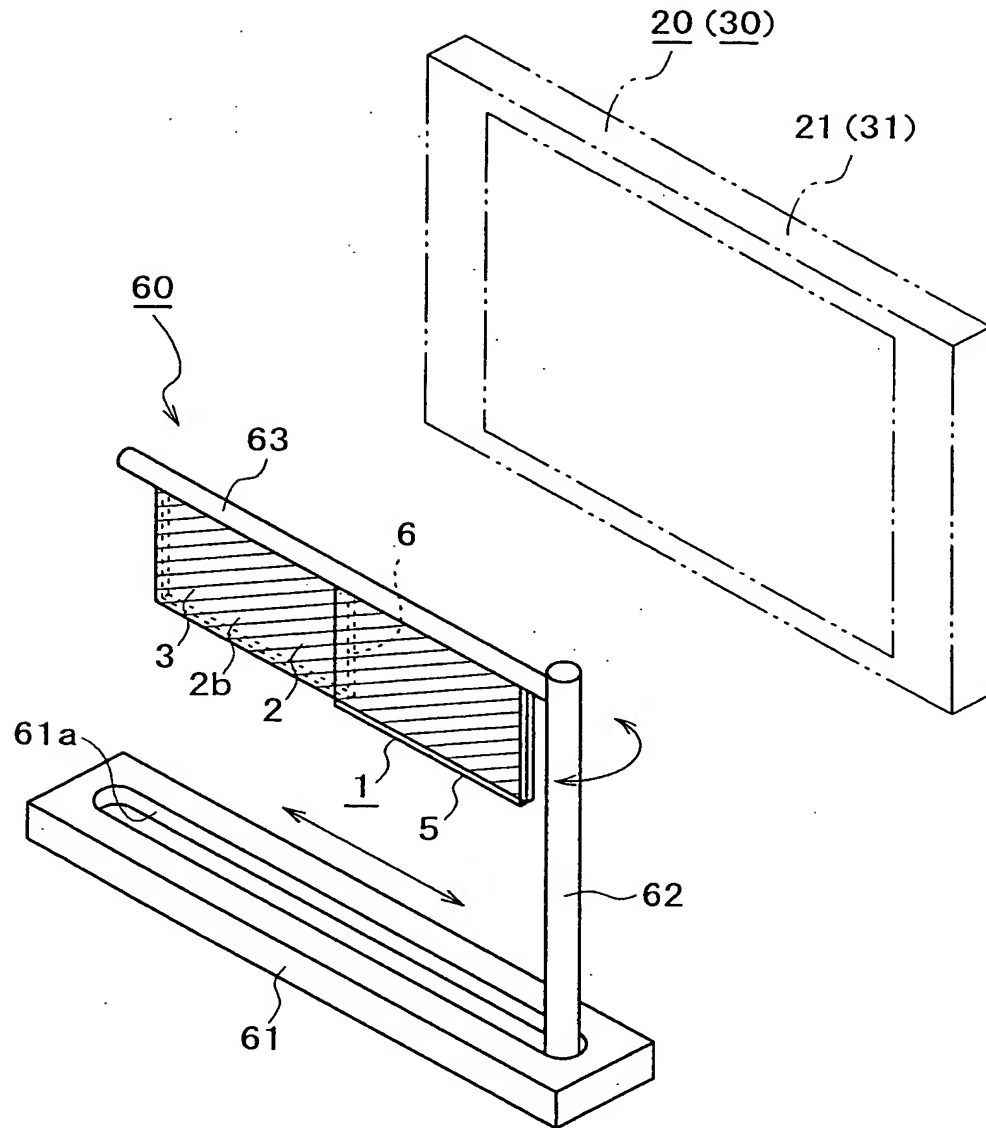



20/32

FIG. 20



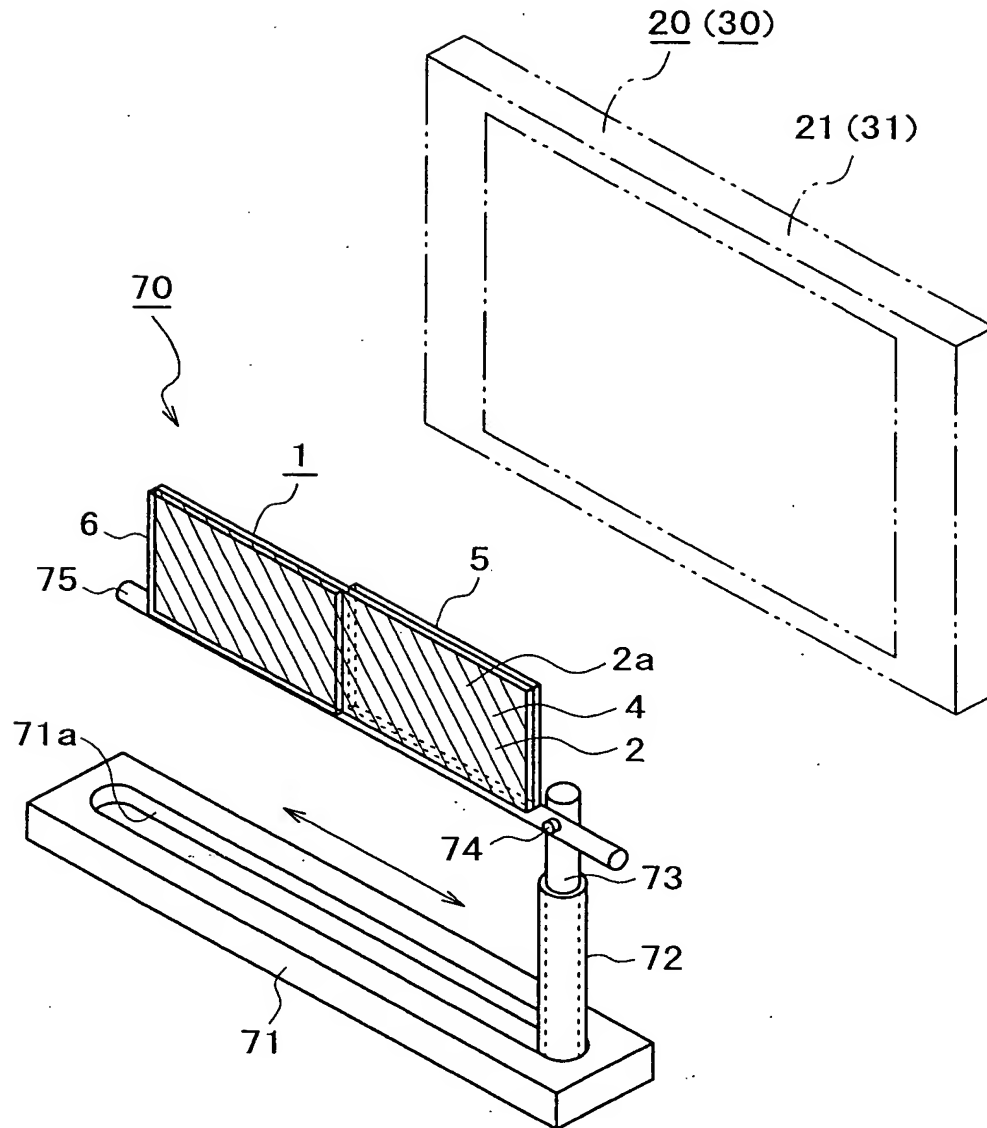


FIG. 21

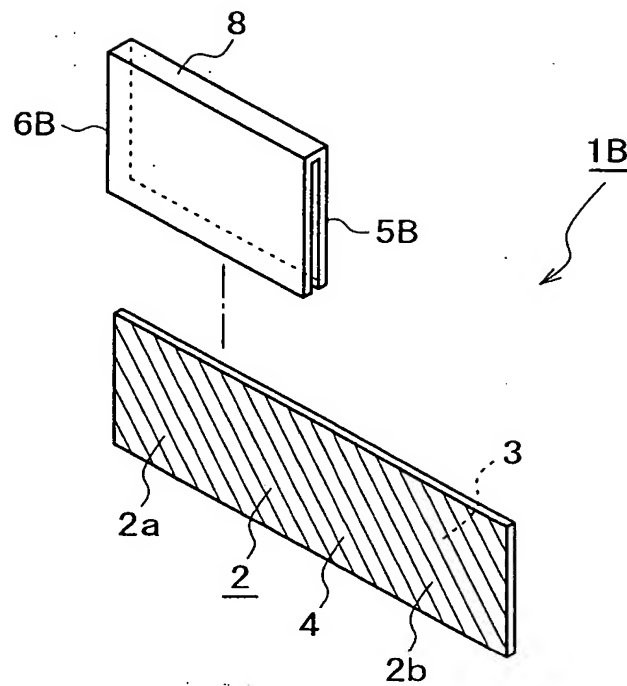


22 / 32

FIG. 22

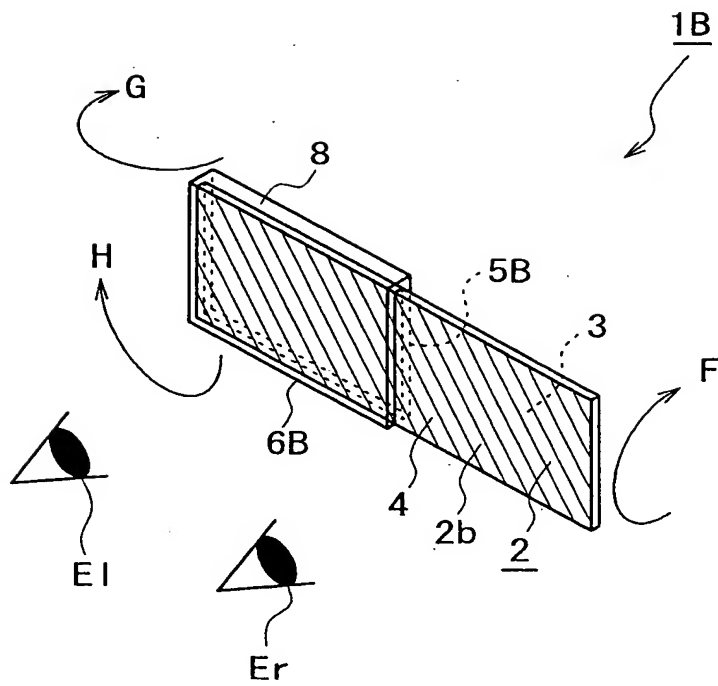


23/32

FIG. 23

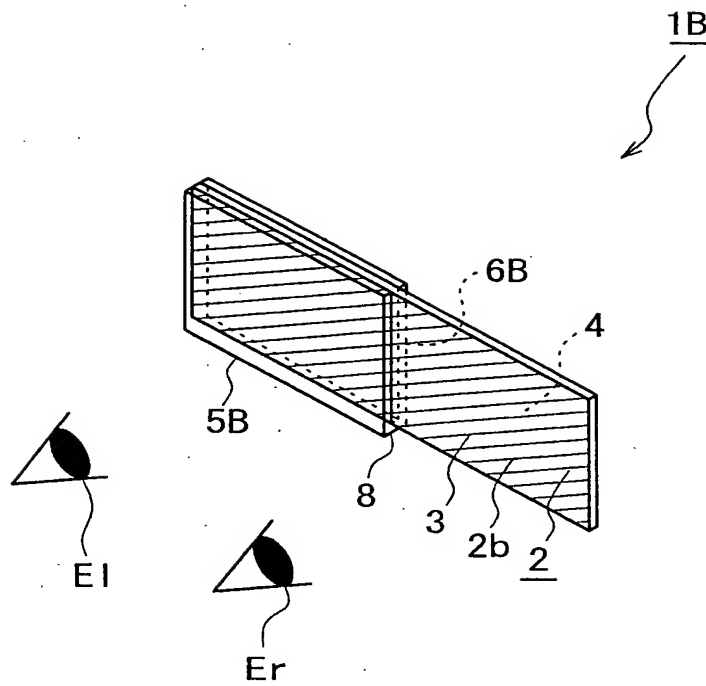

24/32


FIG. 24

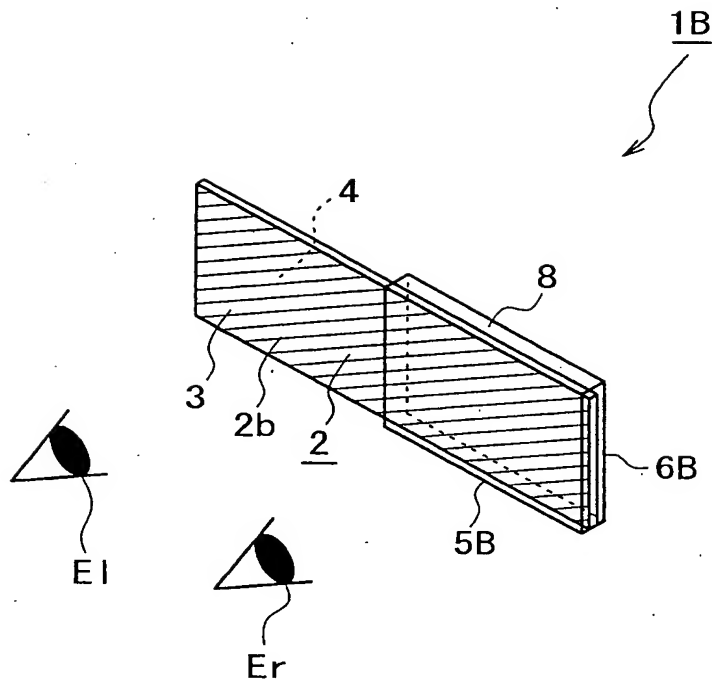



25/32

FIG. 25

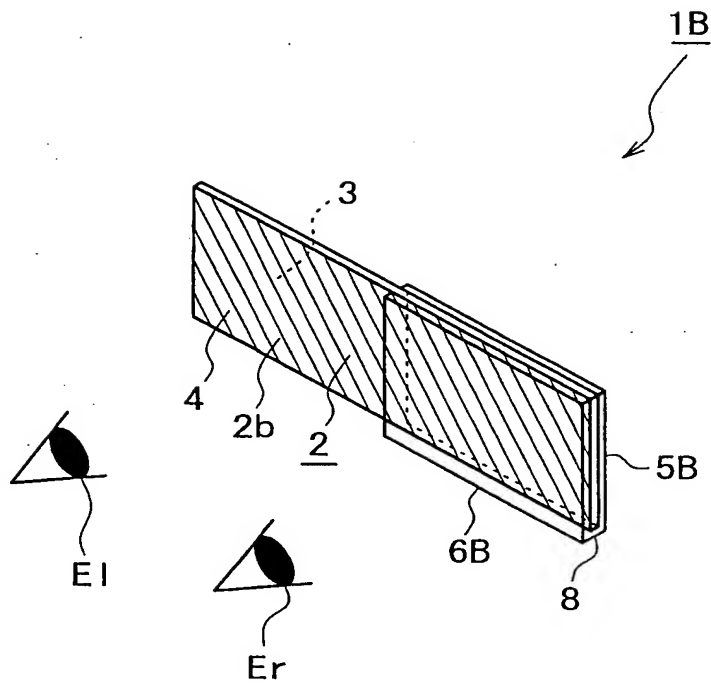



























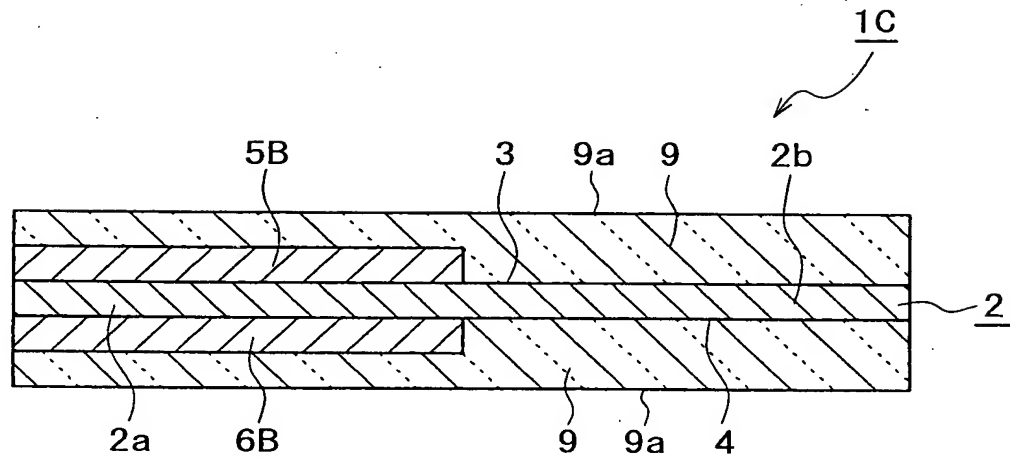
| STEREOSCOPIC IMAGE DISPLAY APPARATUS  |  |   |   |  | POLARIZING EYEGLASS DEVICE  |  |   |   |
|---|--|---|---|--|---|--|---|---|
| TYPE I  | TYPE II  | TYPE III  | TYPE IV   |  | SERVICE CONDITION E   | SERVICE CONDITION F  | SERVICE CONDITION G   | SERVICE CONDITION H   |
|    |    |    |    |  |  |  |  |  |
|    |    |    |    |  |   |  |   |   |
|    |    |    |    |  |   |  |   |   |
|  |  |  |  |  |   |  |   |   |
|  |  |  |  |  |   |  |   |   |

FIG. 27


28 / 32

FIG. 28




29/32

FIG. 29

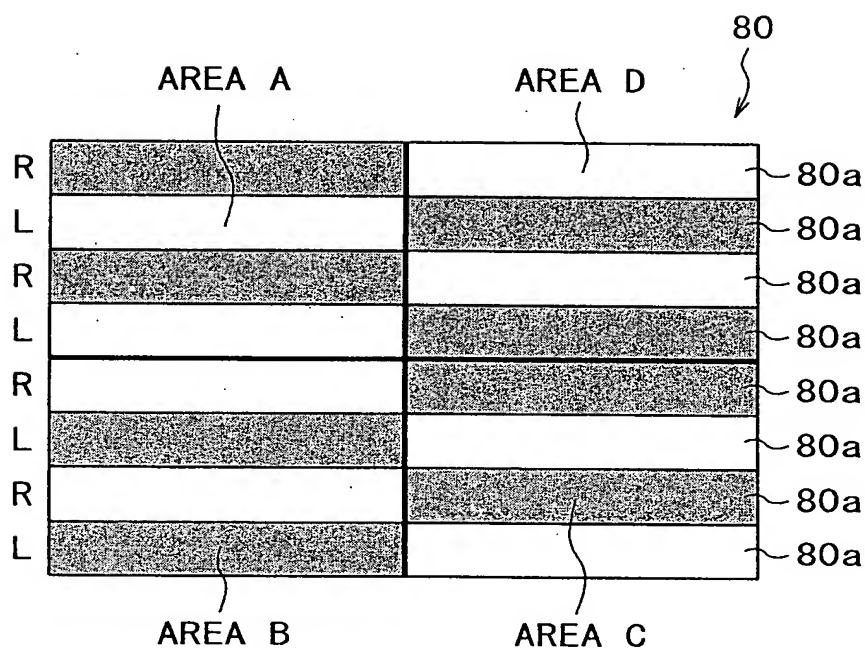


30 / 32

F I G. 3 0

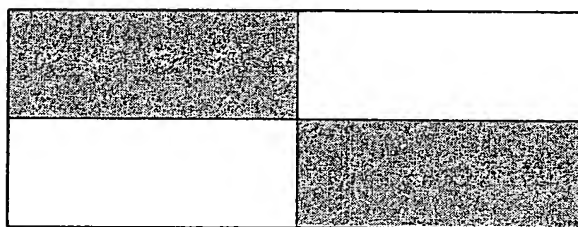


F I G. 3 1

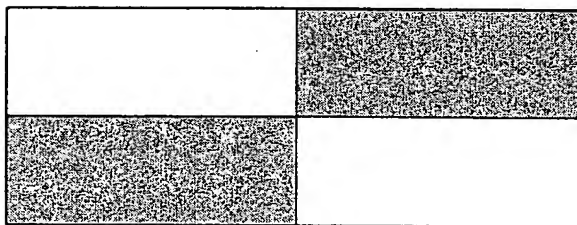

31/32

FIG. 32

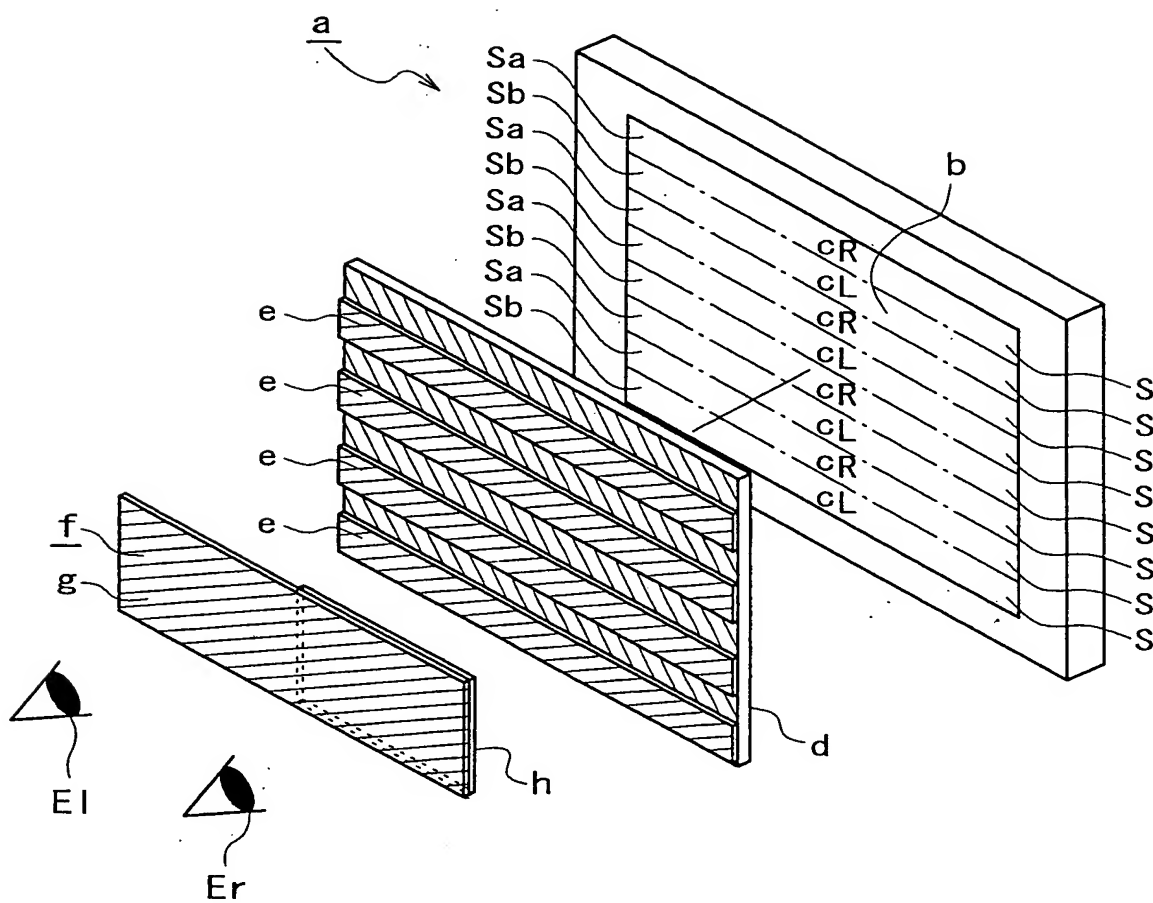

32 / 32

FIG. 33

